

AD-753 001

DETERMINATION OF MOLECULAR INVARIANTS
ALPHA' AND GAMMA'

Samuel Lederman, et al

Polytechnic Institute of Brooklyn

Prepared for:

Army Research Office-Durham

August 1972

DISTRIBUTED BY:

NTIS

National Technical Information Service
U. S. DEPARTMENT OF COMMERCE
5285 Port Royal Road, Springfield Va. 22151

AD753001

72-26

CONTRACT NO. DAH04-69-C-0077
ARPA ORDER NO. 1443, AMENDMENT 2
PROGRAM CODE 9230

DETERMINATION OF MOLECULAR INVARIANTS α' AND γ'

By

Samuel Lederman and Edwin J. Kawecki



Reproduced by
NATIONAL TECHNICAL
INFORMATION SERVICE
U.S. Department of Commerce
Springfield, MA 01151

POLYTECHNIC INSTITUTE OF BROOKLYN

DEPARTMENT


of

AEROSPACE ENGINEERING

and

APPLIED MECHANICS

AUGUST 1972

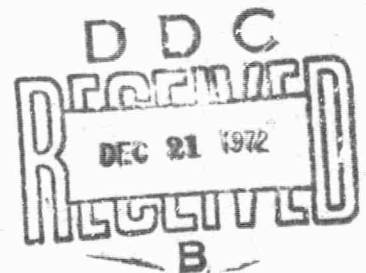

DOCUMENT CONTROL DATA - R & D

(Security classification of title, body of abstract and indexing annotation must be entered when the overall report is classified)

1. ORIGINATING ACTIVITY (Corporate author) Polytechnic Institute of Brooklyn Dept. of Aerospace Eng. & Applied Mechanics Route 110, Farmingdale, New York 11735		2a. REPORT SECURITY CLASSIFICATION Unclassified	
3. REPORT TITLE DETERMINATION OF MOLECULAR INVARIANTS α' AND γ'		2b. GROUP	
4. DESCRIPTIVE NOTES (Type of report and inclusive dates) Research report			
5. AUTHOR(S) (First name, middle initial, last name) Samuel Lederman Edwin J. Kawecki			
6. REPORT DATE August 1972	7a. TOTAL NO. OF PAGES 17 24	7b. NO. OF REFS 8	
8a. CONTRACT OR GRANT NO. DAHCO4-69-C-0077		8b. ORIGINATOR'S REPORT NUMBER(S) PIBAL Report No. 72-26	
9a. PROJECT NO. ARPA Order No. 1442, Amendment 2 Program Code 9E30		9b. OTHER REPORT NO(S) (Any other numbers that may be assigned this report)	
10. DISTRIBUTION STATEMENT Approved for public release; distribution unlimited.			
11. SUPPLEMENTARY NOTES		12. SPONSORING MILITARY ACTIVITY U.S. Army Research Office-Durham Box CM, Duke Station Durham, North Carolina 27706	
13. ABSTRACT The determination of the polarizability invariants and particularly the derivatives of the invariants, the isotropic and anisotropic parts α' and γ' , necessary for the prediction of the Raman scattered intensity are considered. It is shown that a simple method based on the angular dependence of the scattered Raman intensity can be utilized to obtain these invariants, provided the polarization of the incident radiation is known.			

-1a-

KEY WORDS

LINK A

LINK 

LINK C

ROLE

WT

NAME	ROLE
Mr. J. Edgar Hoover	Director
Mr. Clegg	Chief of Bureau
Mr. Glavin	Chief of Bureau
Mr. Ladd	Chief of Bureau
Mr. Nichols	Chief of Bureau
Mr. Rosen	Chief of Bureau
Mr. Tracy	Chief of Bureau
Mr. Carson	Chief of Bureau
Mr. Egan	Chief of Bureau
Mr. Gurnea	Chief of Bureau
Mr. Hendon	Chief of Bureau
Mr. Pennington	Chief of Bureau
Mr. Quinn	Chief of Bureau
Mr. Nease	Chief of Bureau
Mr. Gandy	Chief of Bureau

WT

POLE

WT

Raman scattering
Molecular invariants
Depolarization ratio
Scattering intensity
Angular dependence
Refractive index

-16-

DETERMINATION OF MOLECULAR INVARIANTS α' AND γ'

by

Samuel Lederman and Edwin J. Kawecki

This research was sponsored by the Advanced Research Projects Agency of the Department of Defense and was monitored by the U.S. Army Research Office-Durham, North Carolina under Contract No. DAHCO4-69-C-0077.

Reproduction in whole or in part is permitted for any purpose of the United States Government.

POLYTECHNIC INSTITUTE OF BROOKLYN

Department

of

Aerospace Engineering and Applied Mechanics

August 1972

PIBAL Report No. 72-26

-10-

Approved for public release; distribution unlimited.

TABLE OF CONTENTS

<u>Section</u>		<u>Page</u>
I	Introduction	1
II	Theoretical Background	2
III	Experimental Apparatus	8
IV	Experimental Procedures and Results	8
V	Conclusions	10
VI	References	10

LIST OF ILLUSTRATIONS

<u>Figure</u>		<u>Page</u>
1	Coordinate System Showing the Direction of Laser Irradiation and the Orientation of the Viewing System	12
2	Schematic of the Experimental Apparatus	13
3	Photographic Views of the Experimental Apparatus	14
4	Plot of θ vs. I_{θ}/I_{90} for N_2 and O_2 with Vertically Polarized Laser	15
5	Plot of θ vs. I_{θ}/I_{90} for Oxygen with Horizontally Polarized Laser	16
6	Plot of θ vs. I_{θ}/I_{90} for Nitrogen with Horizontally Polarized Laser	17

LIST OF SYMBOLS

c	velocity of light $2.99793(10)^{10}$ cm/sec.
h	Planck's constant $6.62517(10)^{-27}$ erg.sec.
I	intensity
k	Boltzmann's constant $1.38044(10)^{-16}$ erg/ $^{\circ}$ K
N	number of molecular scatterers
T	temperature
α	isotropic part of the polarizability tensor
α'	spherical (isotropic) part of the change of the polarizability
γ	anisotropic part of the polarizability tensor
γ'	anisotropic part of the change of the polarizability
θ	angle of observation with respect to the incident
μ	reduced mass of the molecule
ν	wave number
ρ	depolarization ratio

Subscripts

h	horizontally polarized incident radiation
o	incident value
s	Stokes component
v	vertically polarized incident radiation
θ	angle between observation and irradiation
\perp	perpendicular
\parallel	parallel

I. INTRODUCTION

The Raman effect has been known and utilized for almost a half century by chemists and physicists interested in molecular structures and chemical, physical thermodynamic and crystallographic properties of matter; these range from force constants, composition, chemical bonds, isomerism, electrolytic dissociation, association to polymerization, exchange interaction, kinetics of fast reactions, structural symmetry or asymmetry, etc. In the last several years, spurred by the development of high power lasers, the application of the Raman effect, due to its unique properties, has found new fields of application¹⁻⁶.

These range from diagnostics of flow fields in fluid dynamics to the remote measurements and monitoring of air pollutants, from temperature measurements of reacting gases to concentration measurements of the products of reactions and combustion. The theory of the Raman effect and Raman spectroscopy on a laboratory level is in a very highly developed state. While the molecular polarizability invariants α' and γ' necessary for the calculation of the equivalent Raman scattering cross-sections are tabulated for a number of molecules, in particular diatomic molecules^{1,7,8}, there is a vast number of molecules for which these invariants are not easily available. A number of methods have been developed for the direct measurement of these

invariants⁷. Some of these methods will be discussed in the next section.

In this work it is shown that it is possible to obtain the polarizability invariants α' and γ' utilizing the angular dependence of the scattered intensity, in particular when one has available a primary illumination source of known polarization.

II. THEORETICAL BACKGROUND

As stated in the Introduction, a number of methods are available for the determination of the polarizability invariants. These are generally based on the experimental determination of the depolarization ratio ρ , defined as the ratio of the intensity of the scattered light polarized perpendicular to the xz plane I_{\perp} , to that polarized parallel to this plane I_{\parallel} , when the incident light approaches along the y-axis and the scattered light is observed at right angles to the y-axis (Fig. 1),

$$\rho = \frac{I_{\perp}}{I_{\parallel}} \quad (1)$$

or, in other words, the ratio of the scattered intensity which is polarized perpendicular to the polarization of the incident radiation to the scattered intensity which is polarized parallel to the polarization of the incident radiation, where all

measurements are made in a direction perpendicular to the propagation direction of the incident radiation. When considering the problem of measuring the state of polarization of Raman scattered radiation by a non-oriented medium such as a gas or liquid, one must perform the averaging process over all possible orientations of scattered radiation. As a result of this process, one arrives at two convenient parts of the derivatives of the polarizability tensor; the first is the isotropic part α' , the other is the anisotropic part γ' . In terms of α' and γ' , the depolarization ratio can be expressed as follows:

$$\rho_{\text{Raman}} = \frac{6\gamma'^2}{45\alpha'^2 + 7\gamma'^2} \quad (2)$$

In a similar fashion, the depolarization ratio of Rayleigh scattered radiation is given by

$$\rho_{\text{Rayleigh}} = \frac{6\gamma^2}{45\alpha^2 + 7\gamma^2} \quad (3)$$

From Eqs. (2) and (3) and from a measurement of the intensity ratio of $I_{\text{Ram}}/I_{\text{Ray}}$ given by

$$\frac{I_{\text{Ram}}}{I_{\text{Ray}}} = \left(\frac{45\alpha'^2 + 7\gamma'^2}{45\alpha^2 + 7\gamma^2} \right) \frac{4}{8\pi^2 \mu_V} \quad (4)$$

and knowing the refractive index of the given gas which permits

the calculation of α from the relation $n-1=2\pi N\alpha$, one can obtain the polarizability invariants α' and γ' .

From the definition of the depolarization ratio, it is evident that at least two measurements are necessary to obtain the same. Here one can distinguish between two basic experimental techniques. One takes cognizance of the polarization of the scattered radiation; the other does not. In order to take account of the polarization of the scattered radiation, one may proceed as follows:

a) One may use unpolarized incident radiation and measure the scattered radiation polarized once in one direction and then polarized perpendicular to the direction of the first measurement.

b) One may use incident radiation which is polarized perpendicular to the direction of observation, and measure scattered radiation polarized parallel to the incident radiation and perpendicular to the incident light polarization.

Since Raman scattered radiation is not polarized, in both the above cases, it is necessary to utilize polarizers for the observation of the scattered radiation. This, of course, complicates the experimental procedure, and it is therefore not the best one could hope for.

The other experimental method for the depolarization ratio measurement does not provide for the measurement of

the polarization of the scattered radiation. Here, too, two procedures are possible. One utilizes incident light polarized parallel and perpendicular to the observation direction and measures the intensity of the scattered radiation, the ratio of which is the depolarization ratio given by Eq. (2). In the other case, one uses incident radiation polarized parallel to the observation direction, and nonpolarized incident light. The ratio of both intensities again provides the polarization ratio. In this case, however, ρ is given by

$$\rho = \frac{6\gamma'^2}{45\alpha'^2 + 13\gamma'^2} \quad (5)$$

While the above procedures provide the required information necessary to obtain the equivalent scattering cross-sections, it is possible to obtain the latter in a much simpler way. One could, for example, obtain the equivalent scattering cross-section of an unknown gaseous or liquid specie by comparing the scattered intensity to the scattered intensity of a specie for which the equivalent scattering cross-section is known, this procedure being followed under the same conditions of illuminating intensity, frequency, pressure, temperature, etc. This procedure can provide information which is sufficient for a great number of applications. However, the polarizability invariants, and the depolarization ratio provide additional

information as to the symmetry of the given molecular structure, the equivalent scattering cross-section, cannot provide.

The Raman scattered intensity as a function of the observation angle θ may be represented for unpolarized primary illumination by

$$I_{\theta} = \frac{\kappa I_0 N(\nu_0 - \nu)^4}{\nu [1 - \exp(-h\nu/kT)]} \{ [45\alpha'^2 + 7\gamma'^2] (1 + \cos^2 \theta) + 6\gamma'^2 \sin^2 \theta \} \quad (6)$$

which reduces for vertically polarized light and normal observation, i.e., normal to the plane formed by the polarization direction and direction of propagation to

$$I_{11} = \frac{\kappa I_0 N(\nu_0 - \nu)^4}{\nu [1 - \exp(-h\nu/kT)]} [45\alpha'^2 + 7\gamma'^2] \quad (7)$$

and for horizontally polarized light to

$$I_{\perp} = \frac{\kappa I_0 N(\nu_0 - \nu)^4}{\nu [1 - \exp(-h\nu/kT)]} [(45\alpha'^2 + 7\gamma'^2) \cos^2 \theta + 6\gamma'^2 \sin^2 \theta]. \quad (8)$$

The depolarization ratio,

$$\rho = \frac{I_{\perp}}{I_{11}} = \frac{(45\alpha'^2 + 7\gamma'^2)}{(45\alpha'^2 + 7\gamma'^2)} \cos^2 \theta + 6\gamma'^2 \sin^2 \theta \quad (9)$$

When the angle of observation is equal to $\pi/2$ with respect to the direction of the incident radiation, Eq. (9)

becomes

$$\rho = \frac{6/7}{45/7 \frac{\alpha'^2}{\gamma'^2} + 1} \quad (10)$$

Since the symmetrical part of the polarizability invariant α' changes only when the molecule is distorted in a totally symmetrical manner, α' will be zero for all vibrations which are not in a totally symmetric specie and the depolarization ratio from Eq. (10) becomes 6/7. On the other hand, all unsymmetrical species will have $\rho < 6/7$ since α' will not vanish. This feature is of importance in identifying totally symmetric vibrations.

Returning now to Eqs. (7) and (8), it is evident that two ratios can be formed. The first, as given in Eq. (9), permits the evaluation of the depolarization ratio ρ , and from it the ratio α'/γ' . The second ratio can be formed by utilizing Eq. (8) above and performing the measurements at two different angles. Thus one may obtain

$$\frac{I_1}{I_2} = \frac{I_{01}}{I_{02}} \frac{[(45\alpha'^2 + 7\gamma'^2)\cos^2\theta_1 + 6\gamma'^2\sin^2\theta_1]}{[(45\alpha'^2 + 7\gamma'^2)\cos^2\theta_2 + 6\gamma'^2\sin^2\theta_2]} \quad (11)$$

It is evident from Eq. (11) that knowing the angles of observation and measuring the scattered radiation intensity I_1 and I_2 , the ratio α'/γ' can be evaluated. This method is quite simple and requires only a simple radiation intensity measurement.

III. EXPERIMENTAL APPARATUS

In order to perform the measurements as indicated above, an apparatus as shown in Fig. 2 was utilized. The apparatus was essentially that of Ref. 3, except that several viewing ports were utilized. These were at $\theta=45^\circ$, 90° , 225° and 270° , as indicated in the figure. A photographic view of the experimental arrangement is shown in Fig. 3. The chamber could be evacuated and pressurized to several atmospheres of pressure. Pressure and vacuum monitoring instrumentation was incorporated in the apparatus. For a complete description, Ref. 3 should be consulted.

A Q-switched ruby laser of 100 megawatt peak power was utilized. Since the chamber was filled with a known gas, and therefore the expected Raman lines were known and no interference or overlapping of frequencies was expected, narrow bandpass filters could be used for these measurements.

IV. EXPERIMENTAL PROCEDURES AND RESULTS

As pointed out above, it is possible to obtain the ratio of d'^2/γ'^2 by simply measuring the intensity of the scattered radiation at two different angles of observation, provided the incident illumination is polarized in the plane of observation (horizontally) and utilizing Eq. (11).

To demonstrate the capability of this method, tests were conducted utilizing gases whose polarizability invariants are well-known and available in the literature. These gases are nitrogen and oxygen. Before, however, attempting to determine the polarizability invariants, a test of the apparatus and the polarization of the lasers was conducted. Since with the laser polarized normal to the plane of observation, no angular dependence is predicted (Eq. (7)), tests were conducted for both N_2 and O_2 in that mode. The results are shown in Fig. 4, where the intensity ratio is plotted as a function of observation angle normalized to the intensity at 90° observation. It is evident from this figure that the experimental results are in good agreement with the theoretical predictions, thus verifying the experimental apparatus and the polarization of the laser.

Having confirmed the operation of the apparatus and the polarization of the laser, tests were conducted for both O_2 and N_2 with the laser polarized in the plane of observation. The scattered intensity as a function of angle of observation was obtained for both species. The results for O_2 and N_2 are shown in Figs. 5 and 6, respectively. The data are presented normalized to the scattered intensity at 90° . In the same figures are also shown the results as given in Refs. 7 and 8.

As can be noted from these figures, the data obtained in this work appear to agree reasonably well with those of Ref. 7. Some scatter of the data is to be expected in view of the single pulse operation of the laser and some minor difficulties in monitoring accurately the primary pulse power during these experiments.

In Table I, the ratio of $(\frac{\alpha'}{\gamma})^2$ as obtained in this work and in Refs. 7 and 8 are shown.


V. CONCLUSIONS

In view of the above experimental results, it may be concluded that the method of obtaining the polarizability invariants utilizing the angular dependence is capable of providing reasonably reliable data quickly, easily and economically, without the need of complicated experimental apparatus and complicated procedures.

VI. REFERENCES

1. Hertzberg, G.: Molecular Spectra and Molecular Structure. Vols. I and II, D. Van Nostrand and Co., Inc. New York, 1963.
2. Symanski, H.: Raman Spectroscopy. Plenum Press, New York, 1967.

3. Widhopf, G.F. and Lederman, S.: Specie Concentration Measurements Utilizing Raman Scattering of a Laser Beam. Polytechnic Institute of Brooklyn, PIBAL Report No. 69-46, AD 701343, November 1969; also, Specie Concentration Measurements Utilizing Laser Induced Raman Scattering, AIAA J., 9, 2, pp. 309-316, February 1971.
4. Lederman, S.: Molecular Spectra and the Raman Effect - A Short Review. Polytechnic Institute of Brooklyn, PIBAL Report No. 71-15, AD 728164, June 1971.
5. Lederman, S.: The Application of the Raman Effect to Remote Monitoring of Air Pollutants. Polytechnic Institute of Brooklyn, PIBAL Report No. 71-29, September 1971.
6. Leonard, D.A.: Observation of Raman Scattering from the Atmosphere Using a Pulsed Nitrogen Laser. Nature, 216, 1967.
7. Yoshino, T. and Bernstein, H.J.: Intensity in the Raman Effect. VI. The Photoelectrically Recorded Raman Spectra of Some Gases. J. Molecular Spectroscopy, 2, 1958.
8. Stansbury, E.J., Crawford, M.F. and Welsh, H.L.: Determination of Rates of Change of Polarizability from Raman and Rayleigh Intensities. Canadian J. Phys., 31, 1953.

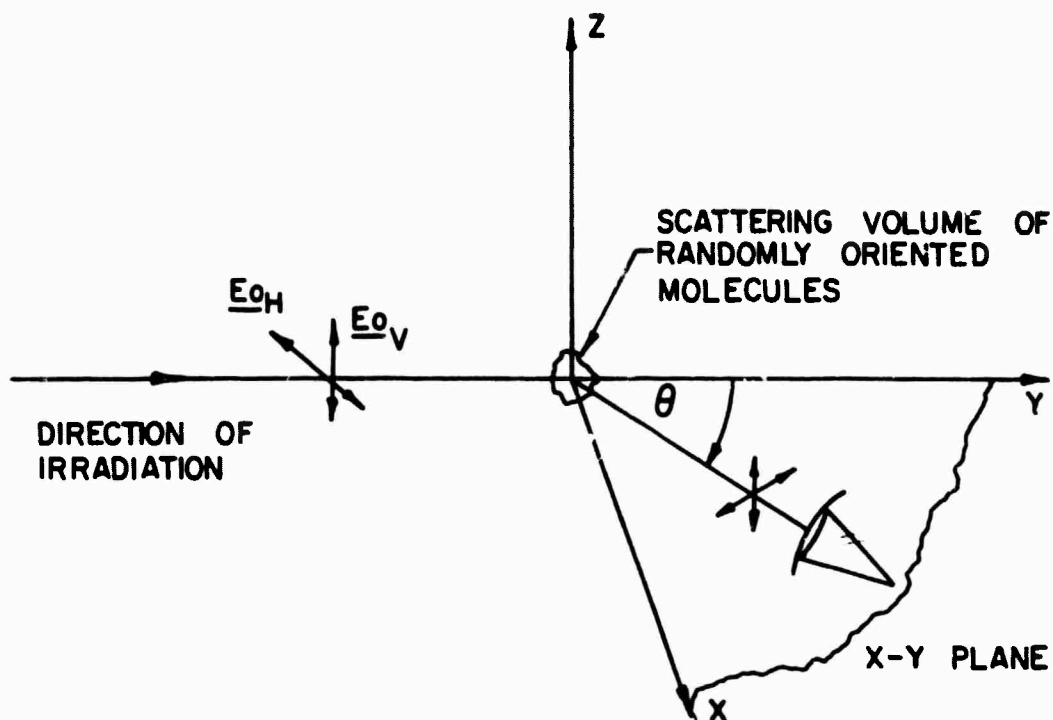

- ()_V - VERTICALLY POLARIZED RADIATION (Y-Z PLANE)
 ()_H - HORIZONTALLY POLARIZED RADIATION (X-Y PLANE)

FIG. 1 COORDINATE SYSTEM SHOWING THE DIRECTION OF LASER IRRADIATION AND THE ORIENTATION OF THE VIEWING SYSTEM



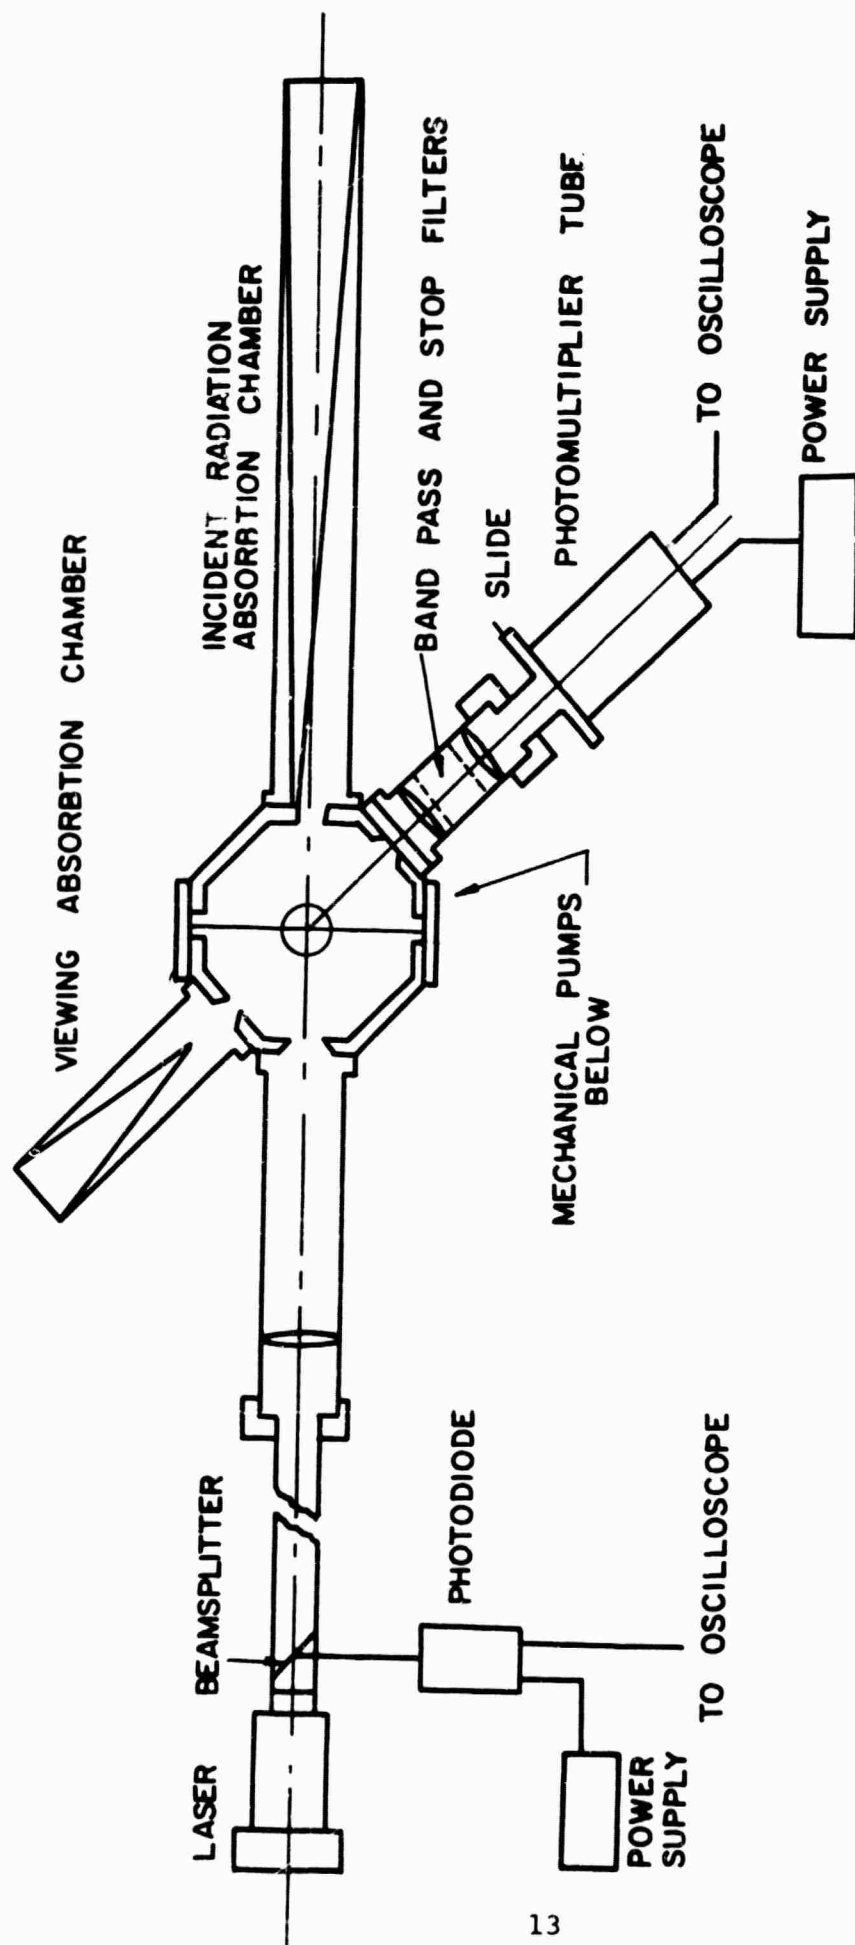


FIG. 2 SCHEMATIC OF THE EXPERIMENTAL APPARATUS

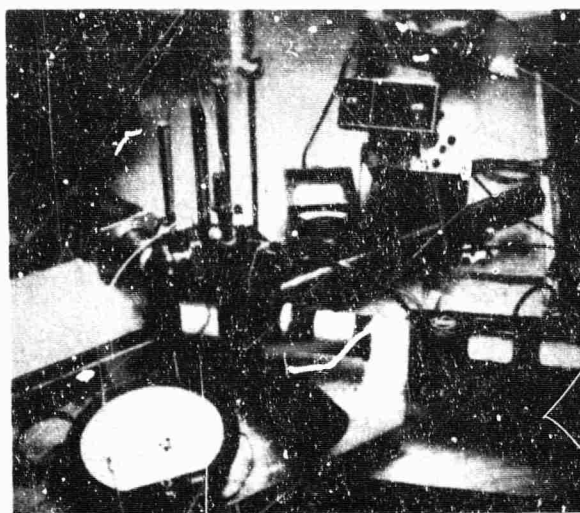

SCATTERING CHAMBER, PHOTOMULTIPLIER TUBE
WITH SUPPORTING EQUIPMENT

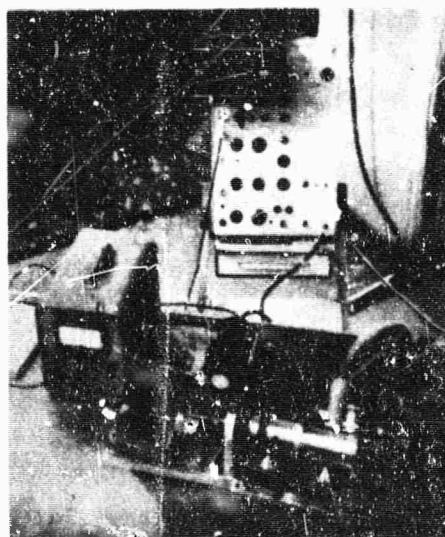

LASER SYSTEM

FIG.3 PHOTOGRAPHIC VIEWS OF THE EXPERIMENTAL
APPARATUS

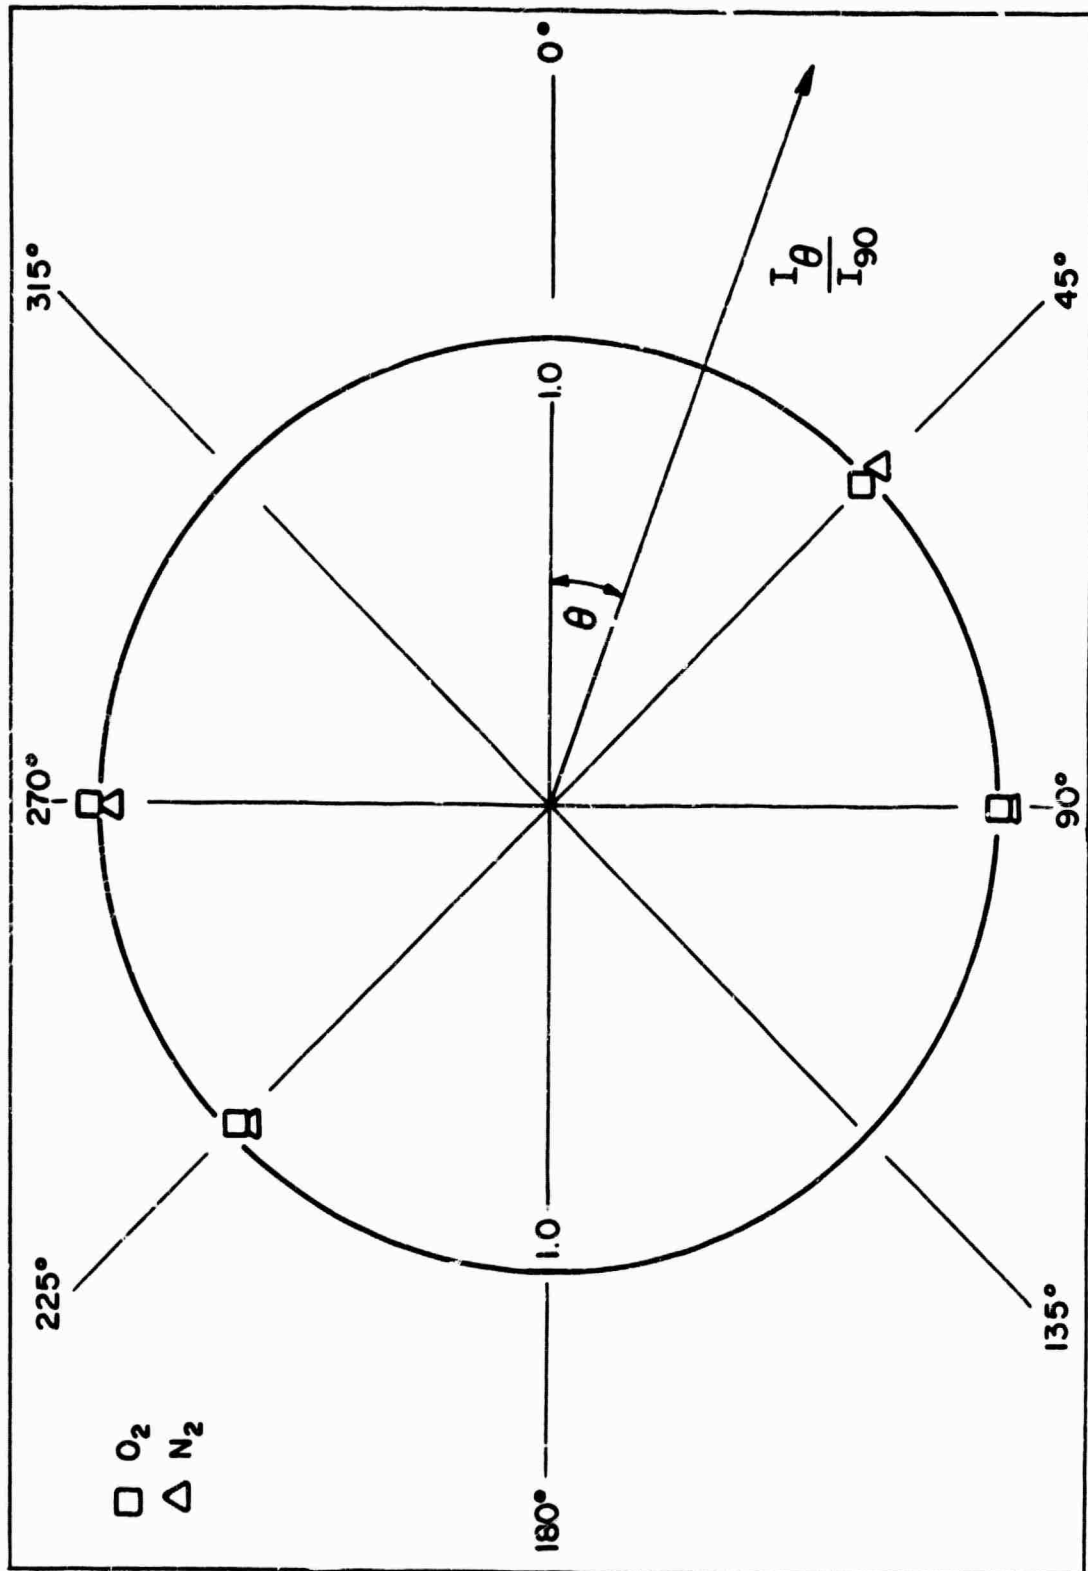


FIG. 4 PLOT OF θ VS. I_θ / I_{90} FOR N_2 AND O_2 WITH VERTICALLY POLARIZED LASER

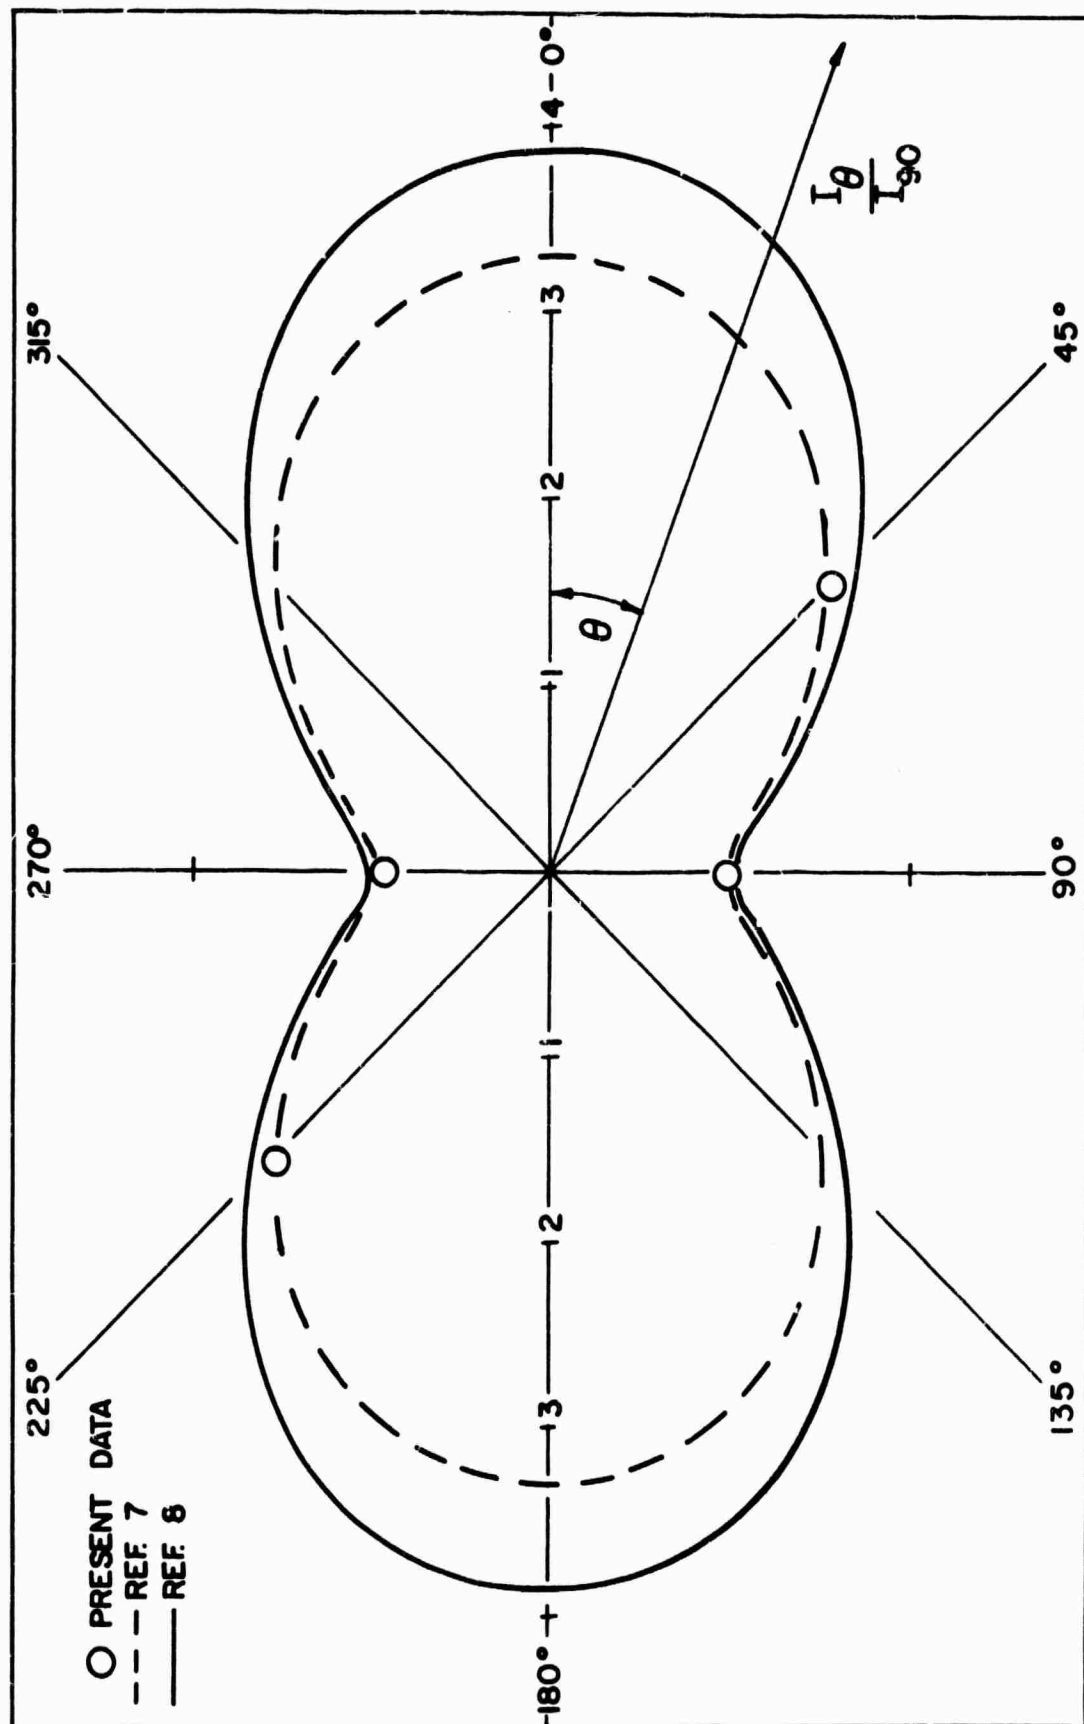


FIG. 5 PLOT OF θ VS. I_{θ} / I_{90} FOR OXYGEN WITH HORIZONTALLY POLARIZED LASER

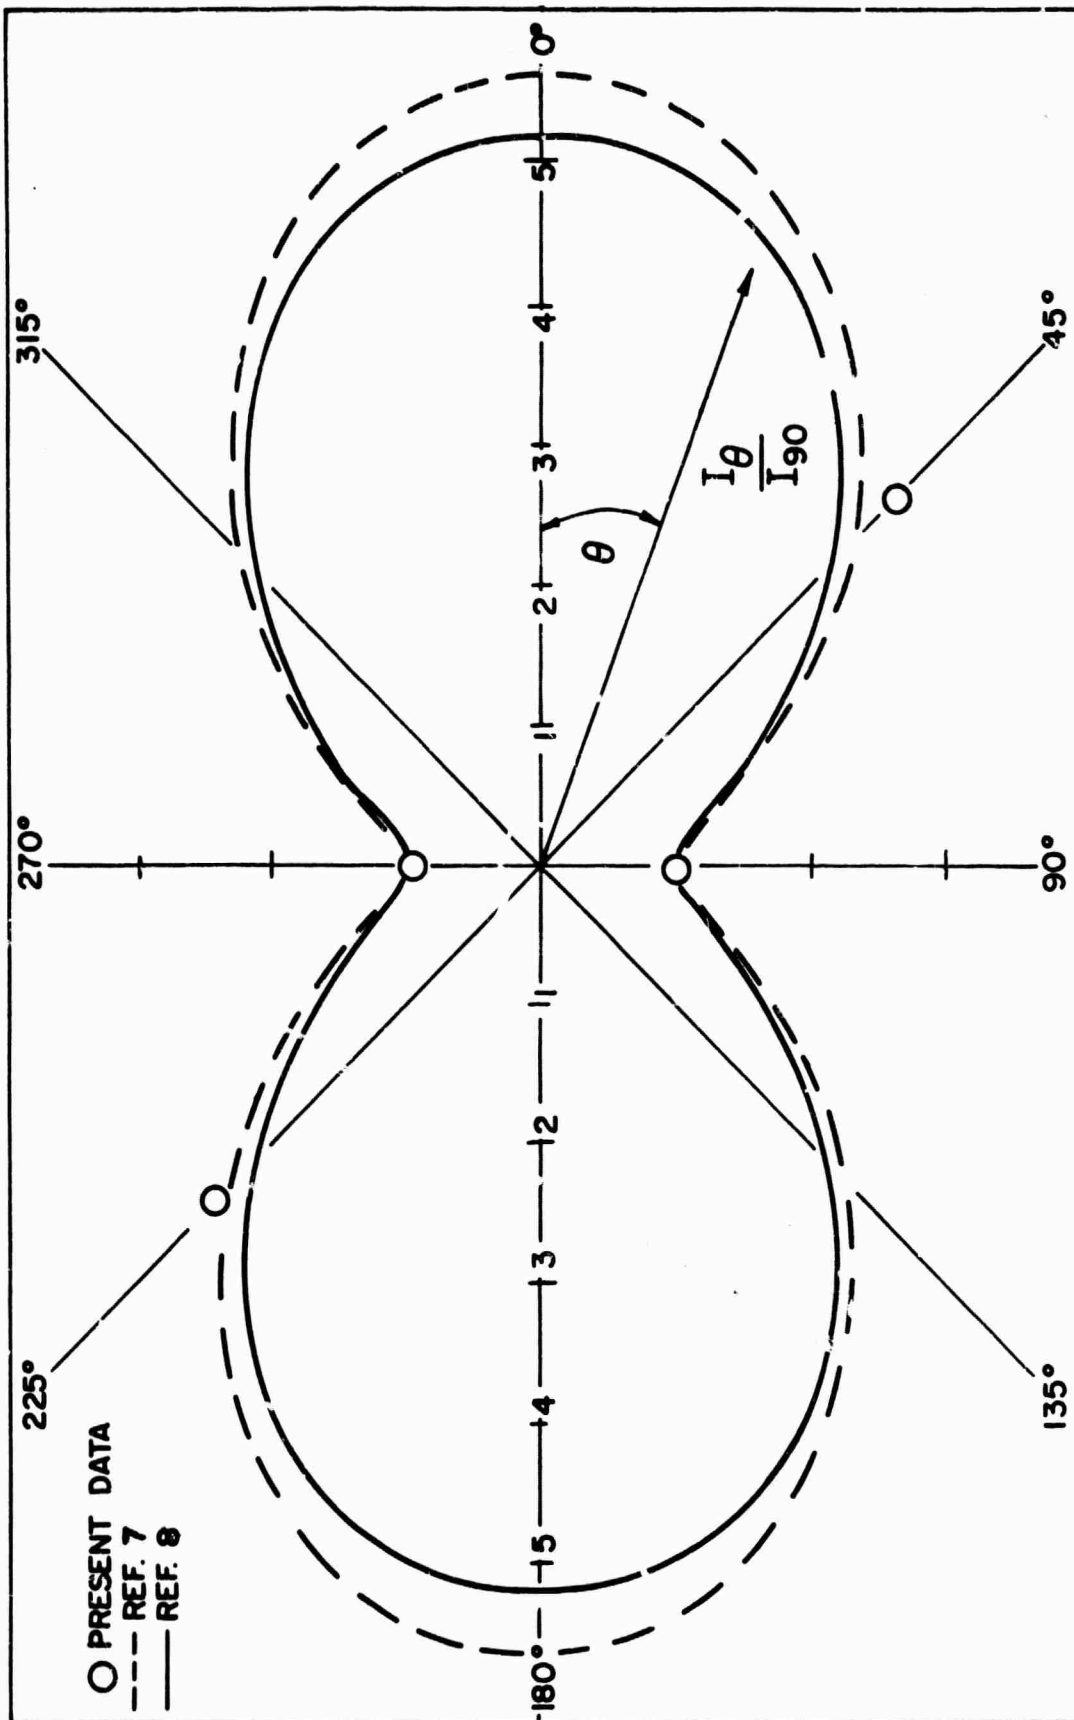


FIG. 6 PLOT OF θ VS. I_{θ} / I_{90} FOR NITROGEN WITH HORIZONTALLY POLARIZED LASER